



JRC VALIDATED METHODS, REFERENCE METHODS AND MEASUREMENTS REPORT

Event-specific Method for the Quantification of Maize MON 95379 Using Real-time PCR

Validation Report

Zaoui X., Sacco M. G., Savini C., Mazzara M.,
Vincent U.

European Union Reference Laboratory for
Genetically Modified Food and Feed

2022

This publication is a Validated Methods, Reference Methods and Measurements by the Joint Research Centre (JRC), the European Commission's science and knowledge service. It aims to provide evidence-based scientific support to the European policymaking process. The contents of this publication do not necessarily reflect the position or opinion of the European Commission. Neither the European Commission nor any person acting on behalf of the Commission is responsible for the use that might be made of this publication. For information on the methodology and quality underlying the data used in this publication for which the source is neither Eurostat nor other Commission services, users should contact the referenced source. The designations employed and the presentation of material on the maps do not imply the expression of any opinion whatsoever on the part of the European Union concerning the legal status of any country, territory, city or area or of its authorities, or concerning the delimitation of its frontiers or boundaries.

Contact information

Name: EURL GMFF

Email: JRC-EURL-GMFF@ec.europa.eu

EU Science Hub

<https://joint-research-centre.ec.europa.eu>

JRC130976

Ispra: European Commission, 2022

© European Union



The reuse policy of the European Commission documents is implemented by the Commission Decision 2011/833/EU of 12 December 2011 on the reuse of Commission documents (OJ L 330, 14.12.2011, p. 39). Unless otherwise noted, the reuse of this document is authorised under the Creative Commons Attribution 4.0 International (CC BY 4.0) licence (<https://creativecommons.org/licenses/by/4.0/>). This means that reuse is allowed provided appropriate credit is given and any changes are indicated.

For any use or reproduction of photos or other material that is not owned by the European Union permission must be sought directly from the copyright holders.

How to cite this report: Zaoui X., Sacco M. G., Savini C., Mazzara M., Vincent U. "Event-specific Method for the Quantification of Maize MON 95379 Using Real-time PCR". European Union Reference Laboratory for GM Food and Feed, Joint Research Centre, 2022. JRC130976. <http://gmo-crl.jrc.ec.europa.eu/StatusOfDossiers.aspx>



Event-specific Method for the Quantification of Maize MON 95379 Using Real-time PCR

Validation Report

10/10/2022

European Union Reference Laboratory for GM Food and Feed

Executive Summary

In line with its mandate ⁽¹⁾ the European Union Reference Laboratory for GM Food and Feed (EURL GMFF), in collaboration with the European Network of GMO Laboratories (ENGL), validated an event-specific real-time polymerase chain reaction (qPCR) method for detecting and quantifying maize event MON 95379 (unique identifier MON-95379-3). The validation study was conducted according to the EURL GMFF validation procedure [<http://gmo-crl.jrc.ec.europa.eu/guidancedocs.htm>] and the relevant internationally accepted guidelines ⁽²⁻⁶⁾.

In accordance with current EU legislation ⁽⁷⁾, Bayer Agriculture BV provided the detection method and the positive and negative control samples (genomic DNA from seeds of MON 95379 maize as positive control DNA, and genomic DNA from seeds of conventional maize as negative control DNA). The EURL GMFF verified the method performance data provided by the applicant, where necessary experimentally, prepared the validation samples (calibration samples and blind samples at different GM percentage [copies GM/total maize haploid genome copies]), organised an international collaborative study and analysed the results.

The EURL GMFF in-house verification and the collaborative study confirmed that the method meets the method performance requirements as established by the EURL GMFF and the ENGL, in line with the provisions of Annex III-3.C.2 to Regulation (EU) No 503/2013 ⁽⁷⁾, and it fulfils the analytical requirements of Regulation (EU) No 619/2011 ⁽⁸⁾. This validation report is published at <http://gmo-crl.jrc.ec.europa.eu/StatusOfDossiers.aspx>.

Content

EXECUTIVE SUMMARY	1
CONTENT	2
1. INTRODUCTION	4
2. DOSSIER RECEPTION AND ACCEPTANCE (STEP 1)	4
3. SCIENTIFIC ASSESSMENT AND BIOINFORMATICS ANALYSIS (STEP 2)	4
3.1. SPECIFICITY ASSESSMENT CONDUCTED BY THE APPLICANT	5
3.2. SPECIFICITY ASSESSMENT CONDUCTED BY THE EURL GMFF.....	5
3.3. VERIFICATION OF THE ENGL ACCEPTANCE PARAMETERS	6
3.4. DNA EXTRACTION	8
4. MATERIALS AND METHOD	9
4.1. SAMPLES	9
4.2. METHOD FOR THE PCR ANALYSIS.....	9
4.3. EURL GMFF EXPERIMENTAL TESTING (STEP 3).....	10
4.3.1. <i>Determination of the zygosity ratio in the positive control sample</i>	10
4.3.2. <i>In-house verification of the method performance against ENGL method acceptance criteria</i>	11
4.4. INTERNATIONAL COLLABORATIVE STUDY (STEP 4).....	12
4.4.1. <i>List of participating laboratories</i>	13
4.4.2. <i>Real-time PCR equipment used in the study</i>	14
4.4.3. <i>Materials used in the international collaborative study</i>	14
4.4.4. <i>Design of the collaborative study</i>	15
4.4.5. <i>Deviations reported from the protocol</i>	15
5. RESULTS	15
5.1. EURL GMFF EXPERIMENTAL TESTING.....	15
5.1.1. <i>Zygosity ratio in the positive control sample</i>	15
5.1.2. <i>In-house verification of method performance against ENGL method acceptance criteria</i>	16
5.2. RESULTS OF THE INTERNATIONAL COLLABORATIVE STUDY.....	19
5.2.1. <i>PCR efficiency and linearity</i>	19
5.2.2. <i>GMO quantification</i>	20
5.2.3. <i>Method performance requirements</i>	21
6. COMPLIANCE OF THE METHOD FOR DETECTION AND QUANTIFICATION OF EVENT MON 95379 WITH THE REQUIREMENTS OF REGULATION (EU) NO 619/2011	23
7. CONCLUSION	24
8. REFERENCES	24
ANNEX 1: EVENT-SPECIFIC METHOD FOR THE QUANTIFICATION OF MAIZE MON 95379 BY REAL-TIME PCR	26

Quality assurance

The EURL GMFF is ISO 17025:2017 accredited [certificate number: Belac 268 TEST (Flexible Scope for determination of Genetically Modified content in % (m/m) and % (cp/cp) in food and feed by DNA extraction, DNA identification and Real-time PCR and for determination of Genetically Modified content in % (cp/cp) in food and feed by DNA extraction and digital PCR)].

The original version of the document containing evidence of internal checks and authorisation for publication is archived within the EURL GMFF quality system.

Address of contact laboratory:

European Commission
Directorate General Joint Research Centre
Directorate F – Health, Consumers and Reference Materials
European Union Reference Laboratory for GM Food and Feed
Food & Feed Compliance (F.5)
Via E. Fermi, 2749. TP201
I-21027 Ispra (VA), Italy

Functional mailbox: JRC-EURL-GMFF@ec.europa.eu

1. Introduction

In line with Regulation (EC) No 1829/2003 ⁽¹⁾, Bayer Agriculture BV provided the EURL GMFF with an event-specific method for detection and quantification of maize event MON 95379 (unique identifier MON-95379-3) together with genomic DNA as positive and negative control samples.

The dossier was found complete (step 1 of the EURL GMFF validation procedure) and the scientific dossier assessment (step 2) concluded that the reported method performance characteristics, assessed against the ENGL method acceptance criteria ⁽⁹⁾, allowed moving the method forward to step 3 of the procedure (experimental testing), where the EURL GMFF verified the purity of the control samples provided and conducted an in-house testing of samples and method.

The positive and negative control DNA, submitted in accordance with Art 5(3)(j) and Article 17(3)(j) of Regulation (EC) No 1829/2003, were found of good quality.

Step 3 was completed with the conclusion that the method could be submitted to the collaborative study (step 4). This study confirmed that the method is well suited for quantifying genomic DNA of GM maize MON 95379, appropriately extracted from food or feed, down to a GM content level of 0.1 % m/m.

The preparation of the report (step 5) was aligned with the timeline communicated by EFSA for its risk assessment.

2. Dossier reception and acceptance (step 1)

Bayer Agriculture BV submitted the identification and quantification method, data demonstrating its adequate performance when applied to genomic DNA extracted from maize MON 95379 GM event and from non GM maize, and the corresponding positive and negative control DNA samples.

The dossier was found to be complete and was thus moved to step 2.

3. Scientific assessment and bioinformatics analysis (step 2)

Documentation and data supplied by the applicant were evaluated by the EURL GMFF for compliance with the ENGL method acceptance criteria.

The specificity of the event-specific assay was verified by the applicant and confirmed by the EURL GMFF by means of bioinformatics analysis, on the basis of the sequence data provided by the applicant.

3.1. Specificity assessment conducted by the applicant

The specificity of the event-specific assay was assessed by the applicant in real-time PCR reactions, according to the method described in Annex 1 (Tables 1, 2, 3 and 4), using at least 2500 haploid genome copies per reaction extracted from:

oilseed rape Ms1, Ms8, Rf1, Rf2, Rf3, Topas19/2, T45, RT73, MON 88302, 73496; **soybean** A2704-12, A5547-127, FG72, MON 89788, MON 87701, MON 87708, MON 87751, 356043, 305423, BPS-CV127-9, MON 87769, MON 87705, DAS 68416-4, DAS-81419-2, DAS-44406-6, 40-3-2; **maize** T25, Bt176, Bt11, MON 87429, MON 87403, MON 87411, MON 87419, MON 87427, MON 87460, MON 810, GA21, MON 863, TC1507, 3272, 5307, MIR604, MIR162, DAS-59122, 98140, MON 88017, MON 89034, DAS-40278-9, NK603, MZHG0JG, VCO-01981-5, DP-004114-3; **cotton** LLCotton25, T304-40, GHB614, GHB119, MON 1445, MON 531, MON 15985, MON 88701, MON 88702, MON 88913, 281-24-236 x 3006-210-23, COT102; **potato** EH92-527-1, AM04-1020, AV43-6-G7; **alfalfa** J101, J163, KK179; **sugar beet** H7-1; **rice** LLRICE62 and conventional oilseed rape, conventional soybean, conventional maize, conventional cotton, conventional potato, conventional alfalfa, conventional sugar beat, conventional rice, and conventional wheat. According to the method developer the MON 95379 assay did not react with any sample except the positive control.

In addition, the applicant performed an in-silico specificity analysis by using the amplicon sequence as a query for BLASTN 2.2.21+ algorithm search against public sequence of National Center for Biotechnology Information (NCBI) and Patent Genbank databases. No sequence showed alignment of both forward and reverse primers or with the full length of the probe.

3.2. Specificity assessment conducted by the EURL GMFF

The detection method spans the 3' insert-to-plant junction in maize MON 95379. The forward primer "MON 95379 primer 1" binds to the insert. The reverse primer "MON 95379 primer 2" binding site was found in the maize genomic border adjacent to the insertion. The probe "MON 95379 probe" binds to the junction between the insert and the 3' genomic region.

The amplicon size is expected to be 87 bp, consistent to what reported by the applicant. The sequence of the amplicon was analysed by BLAST (NCBI) against local copies of the "nt" and "patents" databases, and no significant similarity was found with any other published sequence. In addition, the primers were tested against the sequences of the other GMO events present in the Central Core Sequence Information System (CCSIS) of the JRC, as well as the whole genomes of more than 80 plants (including *Brassica rapa*, *Glycine max*, *Oryza sativa*, *Solanum lycopersicum* and *Zea mays*) using the e-PCR prediction tool (NCBI), and no potential amplicon was identified.

3.3. Verification of the ENGL acceptance parameters

The applicant prepared the calibration curve from a DNA solution (S1) of 10 % maize event MON 95379 genomic DNA (expressed as copy number ratio) which was serially diluted (1:4) in TE 0.1x to obtain solutions S2, S3 and S4, and finally diluted again (1:5) to obtain S5. The parameters (slope, R² coefficient) of five runs of the calibration curve are reported as provided by the applicant (Table 1).

Table 1. Summary of the slope and R² values obtained by the applicant

MON 95379		<i>hmg</i>	
Slope	R ²	Slope	R ²
-3.35	0.99	-3.38	0.99
-3.27	0.99	-3.36	0.99
-3.25	0.99	-3.35	0.99
-3.34	0.99	-3.38	0.99
-3.40	0.99	-3.34	0.99

According to the ENGL method acceptance criteria, the average value of the slope of the standard curve shall range from -3.1 to -3.6 and the R² coefficient shall be ≥ 0.98 .

Table 1 indicates that the slope and R² coefficient of the standard curves for the GM-system (MON 95379) and the maize-specific *high mobility group (hmg)* system (Accession number: GenBank AJ131373.1), as established by the applicant, were within the ENGL acceptance criteria.

Precision and trueness of the method were established by the applicant and fifteen values for each of three first GM levels (expressed as copy number ratio) were provided; for the lowest GM level (0.05 % expressed as copy number ratio), forty-five values were provided. Table 2 reports precision and trueness values for the four GM-levels as provided by the applicant. Both parameters were within the ENGL acceptance criteria (trueness ± 25 %, RSD_r ≤ 25 % across the entire dynamic range).

Table 2. Mean %, precision and trueness values provided by the applicant estimated for single measurements

Expected GM %**	Test results*			
	10	1	0.085	0.05
Measured mean GM %	9.84	0.76	0.064	0.045
Precision (RSD _r %)	5.56	5.43	12.06	19.00
Trueness (bias %)	-1.60	-23.68	-24.95	-11.00

* Numbers are not rounded but are presented as reported by the applicant

** Expressed as copy number ratio

The method met the ENGL acceptance criteria for trueness and precision at the lowest GM level (i.e. 0.05 %, expressed as copy number ratio), which contains 40 copies of MON 95379 in 220 ng of total DNA per reaction. The GM content of this sample is in line with the requirements for testing the Limit of Quantification (LOQ, below or equal to 0.09 % or 50 copies).

The absolute limit of detection (LOD_{abs}) of the MON 95379 event specific and the maize reference real-time PCR methods was assessed by the applicant in 60 PCR replicates at 10, 5 and 1 haploid genome copies per reaction of MON 95379 event and of maize reference DNA. The LOD_{abs} was found to be below 5 haploid genome copies for MON 95379 event-specific method, in line with the ENGL acceptance criteria (below 0.045 % or 25 copies with a level of confidence of 95 %).

The robustness of the method was assessed in eight combinations of the following variations to the method: exact/ \pm 5 % enzyme mix concentration, exact/ \pm 10 % primer concentration, exact/ \pm 10 % probe concentration, \pm 1 μ L master mix volume, \pm 1 °C in annealing temperature. The RSD_r and the trueness calculated for each combination of variations on a sample at the LOQ level (0.085 %) did not exceed 30 %, thus meeting the ENGL acceptance criteria.

Precision and trueness of the method were tested in a transferability study: fifteen values for each of the three GM levels (expressed as copies GM/total haploid genome copies) were provided. Table 2B reports precision and trueness values for the three GM-levels as provided by a laboratory different from the method developer. Both parameters were within the ENGL acceptance criteria (trueness \leq 25 %, RSD_r \leq 25 % across the entire dynamic range).

Table 2B. Mean %, precision and trueness values obtained by the applicant in the transferability study

Expected GM %	Test results		
	10	1	0.085
Measured mean GM %	10	0.95	0.079
Precision (RSD _r %)	4.08	3.36	12.68
Trueness (bias %)	0.01	-5.41	-6.88

3.4. DNA extraction

Genomic DNA was isolated from ground maize seeds, using a modified extraction method from Rogers and Bendich ⁽¹⁰⁾ previously submitted for detection of maize event MON 88017 that has already been validated in-house by the EURL GMFF. The protocol for DNA extraction and a report on testing are published at <https://gmo-crl.jrc.ec.europa.eu/summaries/CRL-VL-16-05-XP-Corrected-version-2.pdf>. According to the experimental data submitted by the applicant, the protocol for DNA extraction generated DNA of suitable quantity and quality for PCR based applications when applied to ground seeds from the maize event MON 95379.

In agreement with the ENGL position, endorsing the modularity principle (see also Annex III to Reg. (EU) No 503/2013), and given the similarity in the matrix, the EURL GMFF considers the above mentioned DNA extraction protocol applicable in the context of the validation of the method for maize event MON 95379.

Annex III to Reg. (EU) No 503/2013 ⁽⁷⁾ requires the applicant to discuss the validity and limitations of the detection methods in the various types of foods and feeds (matrices) that are expected to be placed on the market. To this regard, the applicant stated that “the applicability of the real-time quantitative TaqMan[®] PCR developed for MON 95379 depends on the isolation of sufficient quantity and quality of purified DNA. This method has been tested on DNA extracted from ground seed material. The detection method for MON 95379 should work as far as good quality and intact DNA can be extracted from processed food and feed materials. The provided DNA extraction method is intended for extraction of genomic DNA from seed, which results in primarily high molecular weight DNA indicating that the DNA is intact with limited fragmentation. The processing of maize grain involves varying degrees of mechanical, enzymatic, solvent, heat, acid, pressure treatment, or combinations of these steps. These steps can influence the quality and intactness of DNA contained in the final processed maize products. After extraction of DNA from certain of these processed matrices, the DNA may need additional rounds of processing in order to clean up the DNA and eliminate PCR inhibitors, in order to achieve a quality of genomic DNA that is suitable for PCR ^(11, 12). Regardless of the DNA extraction method employed, studies have shown that the processing steps for maize result in the significant degradation of high molecular weight DNA and failure to PCR amplify products greater than a few 100 base pairs ^(13, 14). Random DNA fragmentation is known to lead to variability in quantitating DNA by qPCR ⁽¹⁵⁾, thus affecting the ability to accurately quantify the presence of a GM event in processed fractions”.

Whenever DNA is extracted from more complex and difficult matrices, a thorough control of the quality of the DNA is recommended in order to ensure that it has the required quality for subsequent PCR analysis.

4. Materials and method

4.1. Samples

The following positive and negative control samples were provided by the applicant to the EURL GMFF in accordance to Regulation (EC) No 1829/2003 Art 2.11^a:

- genomic DNA extracted by the applicant from hemizygous maize seeds and grains harbouring the MON 95379 event (in LH244 × HCL617 genetic background), and
- genomic DNA extracted by the applicant from conventional maize seeds and grains genetically similar to those harbouring the MON 95379 event (also from LH244 × HC617 genetic background).

4.2. Method for the PCR analysis

The PCR method provided by the applicant is an event-specific, quantitative, real-time TaqMan[®] PCR procedure for the determination of the relative content of GM event MON 95379 DNA to total maize DNA. The procedure is a simplex system, in which a maize specific assay targeting the endogenous gene *high mobility group (hmg)*, and the GM target assay for MON 95379 are performed in separate wells. The validated method protocol is published by the EURL GMFF at <http://gmo-crl.jrc.ec.europa.eu/StatusOfDossiers.aspx> and can be found in Annex 1 to this report.

For the detection of GM event MON 95379, an 87 bp fragment of the region spanning the 3' insert-to-plant junction in maize MON 95379 is amplified using specific primers. PCR products are measured during each cycle (real-time) by means of a target-specific oligonucleotide probe labelled with FAM-6 (6-carboxyfluorescein) as reporter dye at its 5' end and TAMRA as fluorescent quencher dye at its 3' end.

For the relative quantification of GM event MON 95379, a maize taxon-specific system amplifies a 79 bp fragment of a maize *high mobility group (hmg)* endogenous gene, using *hmg* gene-specific primers and a *hmg* gene-specific probe labelled with FAM-6 as reporter dye at its 5' end and TAMRA quencher dye at its 3' end.

Standard curves are generated for both the MON 95379 and the *hmg* systems by plotting the C_q values measured for the calibration points against the logarithm of the DNA copy numbers and by fitting a regression line into these data. Thereafter, the standard curves are used to estimate the copy numbers in the test sample DNA by interpolation from the standard curves.

For the relative quantification of event MON 95379 DNA in a test sample, the MON 95379 copy number is divided by the copy number of the maize haploid genome and multiplied by 100 to obtain the percentage value (GM % = MON 95379 / maize haploid genome x 100).

^a Control sample defined as the GMO or its genetic material (positive sample) and the parental organism or its genetic material that has been used for the purpose of the genetic modification (negative sample).

The absolute copy numbers of the calibration curve samples are calculated by dividing the sample DNA mass (nanograms) by the average 1C value for the maize genome (2.73 pg, applicant's source) which is in good agreement with the published value ⁽¹⁶⁾. The copy number values used in the quantification, the GMO contents of the calibration samples, and the total DNA quantity used in the PCR reactions are listed in Table 3.

Note: Numerical values presented in the following tables were rounded keeping two digits for values ≤ 1 , one digit for values between 1 and 10 and no digit for values ≥ 10 , unless otherwise stated. The calculations in the MS Excel files however were done over not rounded data. This approach might create small inconsistencies in the numerical values reported in the tables but it allows a higher precision in the final results.

Table 3. Copy number values of the standard curve samples

Sample code	S1	S2	S3	S4	S5
Total amount of maize DNA in reaction (ng)	250	62	16	3.9	0.78
Target taxon haploid genome copies	91575	22894	5723	1431	286
Target MON 95379 copies	9158	2289	572	143	29

4.3. EURL GMFF experimental testing (step 3)

4.3.1. Determination of the zygosity ratio in the positive control sample

The EURL GMFF verified the zygosity ratio (GM-target to reference target ratio) in the positive control sample to assess the method performance at 0.1 % GM level -expressed as mass fraction of GM material- in relation to the provisions of Reg. (EU) No 619/2011 ⁽⁸⁾.

The copy number of the MON 95379 and of the *hmg* targets in the positive control sample were determined by digital PCR (dPCR) performed on the Bio Rad QX200 Droplet Reader.

Reaction mixes were prepared in order to test the zygosity in five replicates with a final volume of 22 μ L and contained 1X ddPCR Super Mix no dUTP (Bio Rad, Cat. number 64299440), primers and probes at concentrations indicated in the corresponding validated method (MON 95379 primer 1 and 2 at 400 nM each, MON 95379 probe at 200 nM; *hmg* primer 1 and 2 at 300 nM each, *hmg* probe at 160 nM), and 1 μ L of DNA at a concentration of 62.5 ng/ μ L; the DNA concentration was chosen in order to avoid panel saturation (optimal between 200 < positive partitions < 700).

Reaction mixes were loaded into a semi skirt 96-well plate. 'No template controls' were included. After sealing with a sealing aluminium foil using the PX1™ PCR Plate Sealer, the plate was briefly centrifuged (1 min at 1000 rpm) and placed on Bio Rad Automated Droplet Generator (AutoDG).

The instrument added the Automated Droplet Generation oil for Probes (Bio Rad, Cat. number 1864110), generated the droplets in a final volume of 40 µL of the emulsion containing droplets. The AutoDG then transferred all the emulsions into a new semi skirt 96-well plate. The new plate was sealed with a sealing foil with the PX1™ PCR Plate Sealer and run in a Bio Rad C1000 TouchThermal Cycler. The thermal cycling conditions in a final volume of 40 µL were as indicated below.

Step	Temperature (°C)	Time (mm:ss)	Ramp rate	Number of cycles
Polymerase activation	95	10:00	2°C/sec	1
DNA denaturation	94	00:30		40
Annealing/extension	60	01:00		1
Enzyme deactivation	98	10:00		1
Hold	4	Infinite		1

The sealed 96-well plate was then placed in the QX200 Droplet Reader to determine through cytofluorimetry the fraction of fluorescent PCR-positive droplets with respect of the total number of droplets in the original sample by selecting the proper fluorescent dye used. Data analysis and copy number calculations were performed using the Bio-Rad QX200 Droplet Reader Analysis software (QuantaSoft version 1.7.4).

Calculations of means and variances were carried out according to the procedure outlined for random variables in the Annex 4 of the ENGL guidance document 'Verification of analytical methods for GMO testing when implementing interlaboratory validated methods - Version 2' ⁽¹⁷⁾.

4.3.2. In-house verification of the method performance against ENGL method acceptance criteria

The method performance characteristics were verified by quantifying, on a copy number basis, five blind test samples distributed over a range of GM levels (0.06 % - 10 %, see Table 4). The blind test samples were prepared by the EURL GMFF from the genomic DNA provided by the applicant (see 4.1 for details) by mixing MON 95379 maize DNA and non-GM maize DNA.

Table 4. MON 95379 blinded samples GM % contents

MON 95379 GM % (GM copy number/maize haploid genome copy number) x 100
10
5.0
1.0
0.45
0.06

The calibration sample S1 was prepared from the genomic DNA provided by the applicant by mixing the appropriate amount of MON 95379 DNA with control non-GM maize DNA to obtain a 10 % (in copy number ratio related to haploid genome copies) GM sample. Calibration samples S2-S4 were prepared by 4-fold serial dilutions from the S1 sample and sample S5 by a 5-fold serial dilution from the S4 sample (see Table 3).

The experiments were performed on an ABI 7500, a QuantStudio 7 Flex System and a Roche LC480 real-time platform under repeatability conditions and followed the protocol provided by the applicant.

Test samples with GM levels 10 %, 5 %, 1 % and 0.45 % were tested in two real-time PCR runs with two replicates for each GM-level on each plate (total of four replicates per GM-level). The test sample with GM level 0.06 % (in copy number ratio, equal to 0.10 % mass ratio), containing 48 copies of MON 95379 in 220 ng of total DNA per reaction, was tested with 15 replicates in an additional run for each platform. Average values of the slope and of the R² coefficient of the standard curves and method trueness and precision over the dynamic range were evaluated against the ENGL method acceptance criteria.

4.4. International collaborative study (step 4)

The international collaborative trial involved twelve randomly selected laboratories, all being "national reference laboratories, assisting the EURL GMFF for testing and validation of methods for detection", as listed in annex to Regulation (EC) No 120/2014⁽¹⁸⁾ who had expressed their interest in participation. The study was carried out in accordance with the following internationally accepted guidelines:

The IUPAC "Protocol for the design, conduct and interpretation of method-performance studies" (Horwitz, 1995)⁽²⁾

ISO 5725 "Accuracy (trueness and precision) of measurement methods and results", Part 1 and Part 2 (ISO, 1994); ISO 5725-1:1994/Cor 1 (ISO 1998) and ISO 5725-2:1994/Cor 1 (ISO, 2002)⁽³⁻⁶⁾

The objective of the international collaborative study was to verify in experienced laboratories the trueness and precision of the PCR analytical method provided by the applicant and verified in-house by the EURL GMFF.

4.4.1. List of participating laboratories

The twelve laboratories participating in MON 95379 international collaborative study were randomly selected from thirty national reference laboratories (NRL) that offered to participate.

Clear guidance was given to the selected laboratories for strictly following the validation protocol that was provided to them. The participating laboratories are listed in Table 5.

Table 5. Laboratories participating in the validation of the detection method for maize event MON 95379

Laboratory	Country
Center for Agricultural Technology Augustenberg	DE
CREA-DC Sede di Tavazzano	IT
Independent Authority of Public Revenue (IAPR)	GR
Institute of Food Safety, Animal Health and Environment "BIOR"	LV
Italian National Institute of Health (ISS) Food Safety	IT
LUFASpeyer	DE
National Center of Public Health and Analyses (NCPHA)	BG
National Research Institute of Animal Production, National Feed Laboratory	PL
Saxon State Company of Environmental and Agriculture	DE
Service commun des laboratoires du ministère de l'économie et des finances	FR
Wageningen Food Safety Research (WFSR)	NL
Walloon Agricultural Research Centre	BE

4.4.2. Real-time PCR equipment used in the study

Laboratories involved in the collaborative study used the following real-time PCR equipment: one laboratory used ABI 7900HT, two used ABI 7500, one ABI 7500 fast, one ABI 7300, one ABI ViiA 7, one Roche LC 480 II, three ABI QuantStudio 5 and two Biorad CFX 96.

This variability of equipment, with its known potential influence on PCR results, reflects the real-life situation in the control laboratories and provides additional assurance that the method is robust and usable under real conditions.

4.4.3. Materials used in the international collaborative study

For the validation of the quantitative event-specific method, calibration samples (of known GMO content) and blind test samples (of undisclosed GM content = blind samples) were provided by the EURL GMFF to the participating laboratories (for test samples preparation see 4.3.2).

The twelve NRLs participating in the validation study received the following materials:

- ✓ Five calibration samples with known concentrations of GM-event (140 µL of DNA solution each) labelled from S1 to S5 (Table 3).
- ✓ Twenty blinded test DNA samples (70 µL of DNA solution, each at 55 ng/µL) labelled from U1 to U20, representing five GM levels, each in four replicates (Table 4)
- ✓ Reaction reagents:
 - TaqMan® Universal PCR Master Mix (2x), one vial: 8 mL
 - distilled sterile water, one vial: 5 mL
- ✓ Primers and probes (1 tube each) as follows:
 - hmg* taxon-specific assay
 - *hmg* primer 1 (10 µM): 240 µL
 - *hmg* primer 2 (10 µM): 240 µL
 - *hmg* probe (10 µM): 130 µL
 - MON 95379 assay
 - MON 95379 primer 1 (10 µM): 320 µL
 - MON 95379 primer 2 (10 µM): 320 µL
 - MON 95379 probe (10 µM): 160 µL

4.4.4. Design of the collaborative study

Participating laboratories received a detailed validation protocol that included the exact design of the PCR plates, ensuring that on each PCR plate the samples were analysed for the MON 95379 event-specific system and for the *hmg* taxon-specific system. In total, two plates were run by each participating laboratory.

The laboratories prepared the PCR master-mixes for the maize event MON 95379 and the *hmg* assay in accordance with the description provided in the validation protocol. Calibration and test samples were loaded on the PCR plates as per pre-determined plate layout.

The amplification reaction followed the cycling program specified in the protocol. Participants determined the GM % in the test samples according to the instructions and reported the raw data to the EURL GMFF on an Excel sheet that was designed, validated and distributed by the EURL GMFF. All data are stored by the EURL GMFF on a dedicated and protected server.

The EURL GMFF analysed the data against the parameters and the limits set by the ENGL, i.e. trueness, precision, amplification efficiency and linearity.

4.4.5. Deviations reported from the protocol

Eight laboratories reported no deviations from the validation protocol. One laboratory reported a run performed with 40 cycles instead of 45; one laboratory received a primer tube with not enough material (a replacement aliquot was provided); one laboratory reported mixing-up some wells, resulting in one standard sample ran in duplicate (instead of triplicate) and the creation of an outlier; a laboratory reported partially wrong raw data in the reporting form, the issue was solved with no consequences.

5. Results

5.1. EURL GMFF experimental testing

5.1.1. Zygosity ratio in the positive control sample

The results of the digital PCR analysis conducted by the EURL GMFF on the MON 95379 and *hmg* targets to determine the zygosity ratio in the positive control samples are shown in Table 6.

Table 6. Zygoty ratio of the MON 95379 and *hmg* targets in the positive control sample.

Mean ratio (MON 95379/ <i>hmg</i>)	0.59
Standard deviation	0.03
RSD, (%)	5.1
Standard error of the mean	0.01
Upper 95 % CI of the mean	0.61
Lower 95 % CI of the mean	0.58

The mean ratio (MON 95379/*hmg*) equals 0.59. The 95 % confidence interval (CI) spans around 0.60, the expected ratio for a maize control sample, heterozygous for the GM-locus, with a GM parental contribution of female origin and assuming single-copy endogenous gene target. Therefore, the measured mean ratio is not significantly different from the expected ratio, for an $\alpha = 0.05$.

Hence, 0.059 % GM in haploid genome copy numbers corresponds to 0.1 % in mass fraction of GM DNA.

Note: the zygoty ratio herein reported is valid for the positive control sample DNA in the context of the present validation study. It is used to assess the method performance at 0.1 % GM level - expressed as mass fraction of GM material- in relation to the provisions of Reg. (EU) No 619/2011.

When analytical results of official laboratories are primarily expressed as ratio of GM- DNA copy numbers, they shall be translated into mass fraction results by means of the specific conversion factor published in the document "Conversion factors (CF) for certified reference materials (CRM)" (<https://gmo-crl.jrc.ec.europa.eu/guidancedocs.htm>).

5.1.2. In-house verification of method performance against ENGL method acceptance criteria

Test samples with GM levels from 0.45 % to 10 % (expressed in copy number) were tested in two real-time PCR runs with two replicates for each GM-level on each plate (total of four replicates per GM-level). The sample at 0.06 % GM-level (copy number, corresponding to 0.1 % mass fraction) was tested for its precision in quantification in 15 replicates in separate runs (results shown in Table 8, 9 and 10).

Tests were conducted on ABI 7500, a Q7 (QuantStudio 7 Flex System) and a Roche LC480 for robustness.

The standard curve parameters and the results of efficiency, linearity, trueness and precision obtained in the three real-time PCR runs with the test samples are shown in Tables 7A, 7B, 8, 9 and 10.

According to the ENGL method acceptance criteria, the average value of the slope of the standard curve shall range from -3.1 to -3.6 and the R² coefficient shall be ≥ 0.98 . Table 7A and 7B document that the slopes of the standard curves and the R² coefficients were within the limits established by the ENGL. The EURL GMFF in-house results confirm the data provided by the applicant.

Table 7A. Standard curve parameters of the real-time PCR tests, carried out on ABI 7500, Q7 and Roche LC480 to quantify GM-levels in the range 0.45 % to 10 % (copy number) in four replicates each. Slope and R² coefficient values were rounded to two digits.

	MON 95379			<i>hmg</i>		
	Slope	PCR efficiency*	R ²	Slope	PCR efficiency*	R ²
Run A	-3.4	98	1.00	-3.3	99	1.00
Run B	-3.4	98	1.00	-3.4	97	1.00
Run C	-3.4	97	1.00	-3.3	100	1.00
Run D	-3.3	101	1.00	-3.3	99	1.00
Run E	-3.4	99	1.00	-3.3	100	1.00
Run F	-3.4	98	1.00	-3.4	99	1.00

* PCR efficiency (%) is calculated using the formula Efficiency = $(10^{(-1/\text{slope})} - 1) \times 100$

Runs A-B were carried out on ABI 7500; runs C-D were carried out on Q7; runs E and F were carried out on Roche LC480.

Table 7B. Standard curve parameters of the real-time PCR tests, carried out on ABI 7500, Q7 and Roche LC480 to quantify the GM-level 0.06 % (copy number, equal to 0.1 % in mass fraction) in 15 replicates. Slope and R² coefficient values were rounded to two digits.

	MON 95379			<i>hmg</i>		
	Slope	PCR efficiency*	R ²	Slope	PCR efficiency*	R ²
Run G	-3.5	94	1.00	-3.4	98	1.00
Run H	-3.3	103	1.00	-3.3	101	1.00
Run I	-3.4	96	0.99	-3.4	96	1.00

* PCR efficiency (%) is calculated using the formula Efficiency = $(10^{(-1/\text{slope})} - 1) \times 100$

Run G was carried out on ABI 7500; run H was carried out on Q7; run I was carried out on Roche LC480.

According to the ENGL method acceptance criteria the method trueness (measured as bias in % of the target GM level) should be within ± 25 % of the accepted reference value over the entire dynamic range and the precision, expressed as RSD_r % (relative standard deviation of repeatability), should be ≤ 25 %, also over the entire dynamic range.

Tables 8, 9 and 10 show that trueness and precision of quantification were within the limits established by the ENGL for the PCR machines used.

Table 8. Values of trueness and precision as established by the EURL GMFF in its in-house verification using an ABI 7500. GM % in copy/copy haploid genomes.

Target GM-levels %	Measured GM-level %	Bias % of the target GM-level	Precision (RSD_r %)
10	9.4	-5.7	4.5
5.0	4.6	-7.5	5.2
1.0	0.94	-6.2	4.7
0.45	0.37	-17	9.3
0.06	0.06	3.1	16

Table 9. Values of trueness and precision as established by the EURL GMFF in its in-house verification using a Q7. GM % in copy/copy haploid genomes.

Target GM-levels %	Measured GM-level %	Bias % of the target GM-level	Precision (RSD_r %)
10	10	0.40	5.3
5.0	5.0	0.37	1.7
1.0	1.0	1.2	2.8
0.45	0.43	-5.2	3.4
0.06	0.05	-16	16

Table 10. Values of trueness and precision as established by the EURL GMFF in its in-house verification using a Roche LC480. GM % in copy/copy haploid genomes.

Target GM-levels %	Measured GM-level %	Bias % of the target GM-level	Precision (RSD_r %)
10	9.8	-1.8	2.6
5.0	4.7	-6.1	5.6
1.0	0.97	-2.5	3.6
0.45	0.40	-11	5.8
0.06	0.06	4.9	13

5.2. Results of the international collaborative study

5.2.1. PCR efficiency and linearity

The PCR efficiency (%) and R² values (expressing the linearity of the regression) for the standard curve, reported by participating laboratories are displayed in Table 11. The PCR efficiency (%) was calculated from the standard curve slopes using the formula:

$$\text{Efficiency (\%)} = \left(10^{\frac{-1}{\text{slope}}} - 1\right) \times 100$$

Table 11 indicates that the efficiency of amplification for MON 95379 ranges from 91 % to 107 % and the linearity from 0.97 to 1.00; the amplification efficiency for the maize-specific method ranges from 90 % to 100 % and the linearity from 0.99 to 1.00.

Table 11. Values of slope, PCR efficiency and R² obtained during the international collaborative trial. Slope and R² coefficient values were rounded to two digits.

Lab	Plate	MON 95379			<i>hmg</i>		
		Slope	PCR Efficiency (%)	R ²	Slope	PCR Efficiency (%)	R ²
1	A	-3.6	91	0.99	-3.5	94	1.00
	B	-3.4	97	1.00	-3.5	94	1.00
2	A	-3.5	95	1.00	-3.5	94	1.00
	B	-3.4	99	0.99	-3.4	95	1.00
3	A	-3.5	93	1.00	-3.3	100	1.00
	B	-3.4	98	1.00	-3.4	96	1.00
4	A	-3.3	101	1.00	-3.3	99	1.00
	B	-3.3	100	0.99	-3.5	93	1.00
5	A	-3.5	94	0.99	-3.5	92	1.00
	B	-3.5	94	0.99	-3.5	93	1.00
6	A	-3.4	96	0.99	-3.5	94	1.00
	B	-3.5	92	0.99	-3.4	96	1.00
7	A	-3.2	107	0.99	-3.4	96	1.00
	B	-3.4	97	0.99	-3.4	96	0.99
8	A	-3.4	98	1.00	-3.5	93	1.00
	B	-3.4	95	1.00	-3.5	93	1.00
9	A	-3.4	96	1.00	-3.4	95	1.00
	B	-3.4	99	0.99	-3.6	90	1.00
10	A	-3.4	97	1.00	-3.4	98	1.00
	B	-3.4	96	1.00	-3.4	95	1.00
11	A	-3.3	100	1.00	-3.4	96	1.00
	B	-3.3	103	0.97	-3.5	94	1.00
12	A	-3.3	99	1.00	-3.4	95	1.00
	B	-3.4	96	1.00	-3.5	94	1.00
Mean		-3.4	97	1.00	-3.5	95	1.00

The mean PCR efficiency was 97 % for MON 95379 and 95 % for *hmg*. The average R² of the methods was 1.00 for both MON 95379 and *hmg*. Both PCR efficiency and linearity values were within the ENGL acceptance criteria.

These results confirm the appropriate performance characteristics of the methods tested in terms of efficiency and linearity.

5.2.2. GMO quantification

Table 12 reports the values of quantification for the four replicates of each GM level as reported by each of the twelve participating laboratories.


Table 12. GM % values determined by laboratories for test samples

LAB	GMO content (%) *																			
	0.06				0.45				1				5				10			
	REP 1	REP 2	REP 3	REP 4	REP 1	REP 2	REP 3	REP 4	REP 1	REP 2	REP 3	REP 4	REP 1	REP 2	REP 3	REP 4	REP 1	REP 2	REP 3	REP 4
1	0.05	0.06	0.07	0.08	0.41	0.42	0.46	0.47	0.99	1.0	0.99	0.99	4.8	5.1	4.8	4.8	9.5	9.5	9.6	9.5
2	0.07	0.06	0.07	0.06	0.49	0.53	0.54	0.52	1.1	1.2	1.2	1.2	5.6	5.9	5.2	5.8	11	11	11	10
3	0.05	0.05	0.07	0.07	0.44	0.38	0.44	0.42	0.97	0.89	1.0	1.0	2.4	4.3	4.9	4.9	9.9	8.9	9.1	10
4	0.06	0.06	0.06	0.05	0.44	0.47	0.40	0.41	0.98	1.0	1.0	0.96	5.2	5.2	5.1	5.0	10	11	10	10
5	0.06	0.07	0.08	0.07	0.49	0.44	0.45	0.49	1.0	0.99	1.0	1.0	5.1	5.0	5.0	5.0	9.4	10	9.4	9.9
6	0.05	0.06	0.06	0.08	0.35	0.39	0.54	0.59	0.80	1.1	1.1	0.96	4.1	5.3	6.6	4.6	12	5.2	9.6	11
7	0.08	0.10	0.06	0.06	0.58	0.67	0.46	0.46	1.1	1.2	1.1	1.0	4.6	6.5	5.8	5.5	11	11	11	11
8	0.06	0.08	0.07	0.06	0.42	0.46	0.45	0.47	1.0	0.99	1.1	1.0	5.2	5.1	4.9	5.1	10	9.6	9.7	10
9	0.06	0.08	0.07	0.06	0.44	0.58	0.44	0.45	1.1	1.3	1.0	1.1	7.3	5.8	5.2	5.1	10	15	14	10
10	0.06	0.06	0.06	0.06	0.51	0.55	0.47	0.49	1.0	1.1	1.1	1.1	5.3	5.5	5.2	5.2	10	9.9	11	9.8
11	0.05	0.04	0.06	0.06	0.32	0.34	0.43	0.37	0.84	0.71	1.0	0.89	4.1	3.5	5.3	4.6	8.6	9.4	8.1	11
12	0.07	0.06	0.06	0.05	0.46	0.46	0.43	0.42	1.1	1.1	0.95	0.95	5.1	5.3	4.8	4.7	9.8	10	10	9.7

* GMO % = (GMO copy number/maize haploid genome copy number) x 100

A graphical representation of the data reported in Table 12 is provided in Figure 1 showing the relative deviation from the true value for each GM level tested for the participating laboratory. The coloured bars represent the deviation of the GM level measured in % of the true GM level; the green stripes bar on the right represents the mean relative deviation over all data before eliminating outliers for each GM level.

Figure 1. Relative deviation (%) from the true value of GM level *

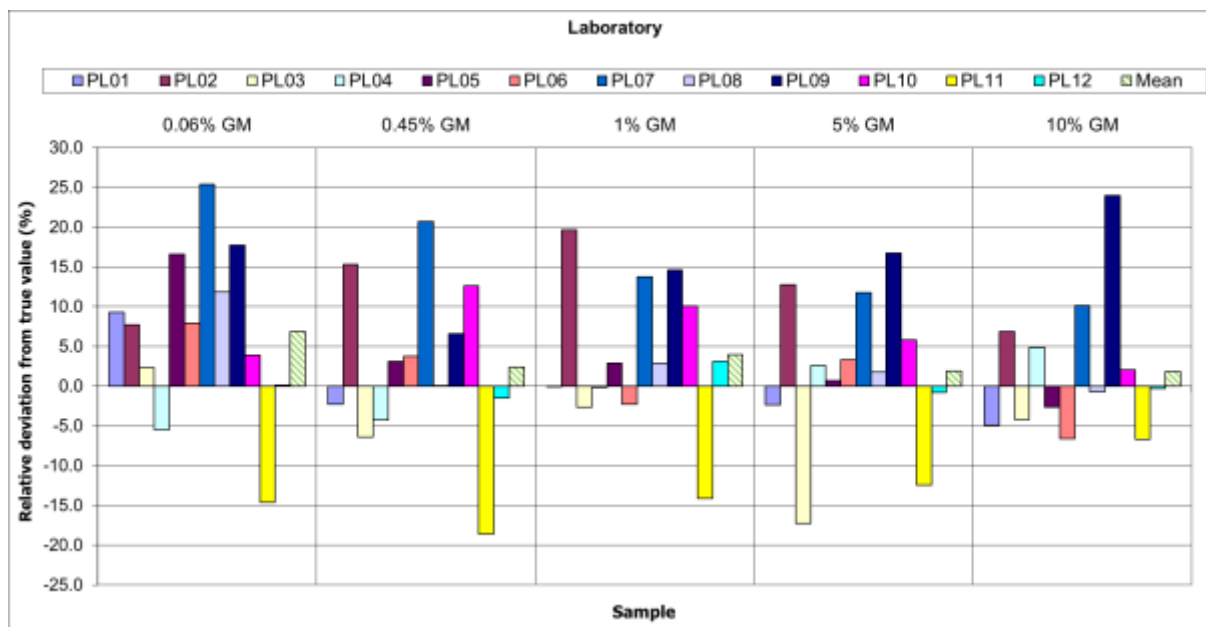

* For PL08 at level 0.45 % a very small relative deviation from the true value was observed and therefore the corresponding histogram does not show in Figure 1. PL = participating laboratory.

Overall, most laboratories' mean relative deviations from the true values were within a maximum of $\pm 25\%$. At every GM-level, eleven laboratories were within the limit. One laboratory overestimated GM-level 0.06 % by more than 25 %. PL02, PL07, PL09, PL10 appear to slightly overestimate values, while PL11 tend to underestimate them; however overall, no clear trend for over- or underestimation was observed.

5.2.3. Method performance requirements

Among the performance requirements established by ENGL and adopted by the EURL GMFF (<http://gmo-crl.jrc.ec.europa.eu/guidancedocs.htm>), repeatability and reproducibility are to be assessed through an international collaborative trial. Table 13 illustrates the estimation of repeatability and reproducibility at the various GM levels tested during the study (see Table 4 for a list of the participant laboratories).

According to the ENGL method performance requirements the relative reproducibility standard deviation (RSD_R), that describes the inter-laboratory variation, should be below 35 % at the target concentration and over the majority of the dynamic range, while it should be below 50 % at the lower end of the dynamic range.

As it can be observed in Table 13, the method satisfies this requirement at all GM levels tested. Indeed, the highest value of RSD_R % is 17 % at the 0.06 % GM level, thus within the acceptance criterion.

Table 13. Summary of validation results for the MON 95379 method, expressed as GM copy numbers in relation to target taxon haploid genome copy numbers.

	Test Sample Expected GMO %				
	0.06	0.45	1.0	5.0	10
Laboratories having returned valid results	12	12	12	12	12
Samples per laboratory	4	4	4	4	4
Number of outliers	0	0	0	0	3
Reason for exclusion *	-	-	-	-	3 C
Mean value	0.06	0.46	1.0	5.1	10
Relative repeatability standard deviation, RSD_r (%)	15	12	7.6	13	3.9
Repeatability standard deviation	0.01	0.05	0.08	0.64	0.39
Relative reproducibility standard deviation, RSD_R (%)	17	15	11	15	6.1
Reproducibility standard deviation	0.01	0.07	0.12	0.74	0.62
Bias** (absolute value)	0.004	0.01	0.04	0.09	0.12
Bias (%)	6.9	2.4	4.0	1.9	1.2

* C = Cochran's test; identification and removal of outliers through Cochran test, according to ISO 5725-2.

** Bias is estimated according to ISO 5725 data analysis protocol.

Table 13 also documents the relative repeatability standard deviation (RSD_r) estimated for each GM level. In order to accept methods for collaborative study, the EURL GMFF and ENGL require that the RSD_r value indicated by the applicant and confirmed by the EURL GMFF through in-house experiments, is below 25 % (see ENGL document "Definition of Minimum Performance Requirements for Analytical Methods of GMO Testing" <http://gmo-crl.jrc.ec.europa.eu/guidancedocs.htm>). As it can be observed from the values reported, the repeatability standard deviation is below 25 % at all GM levels, with the highest value of 15 % at the 0.06 % GM level.

The trueness of the method is estimated using the measures of the method bias for each GM level. According to ENGL method performance requirements, trueness should be ± 25 % across the entire dynamic range. The method satisfies this requirement across the dynamic range tested, with the highest value of bias (%) of 6.9 % at the 0.06 % GM level.

6. Compliance of the method for detection and quantification of event MON 95379 with the requirements of Regulation (EU) No 619/2011

To verify the compliance of the method under validation with the requirements of Regulation (EU) No 619/2011, the following steps were carried out and their outcome is summarised in Table 14:

- at step 2 of the validation process (scientific assessment of the dossier), the EURL GMFF acknowledged that the RSD_r value at the 0.05 % level shown by the applicant's dossier (expressed as copy number ratio) was 19 %, based on forty-five replicates (Table 2), and 13 % based on fifteen replicates in the transferability study (at the 0.085 % level, Table 2B), hence below the maximum value of 25 % required by the ENGL. The EURL GMFF therefore concluded that it could accept the applicant's data on method performance;
- at step 3 of the validation process (experimental testing of samples and methods), the EURL GMFF determined the RSD_r % value at the level of 0.1 % in mass fraction of GM-material (corresponding to 0.06 % expressed in terms of copy number ratio to haploid genome copy numbers). The experiments were carried out under repeatability conditions on fifteen replicates. The RSD_r resulted to range between 13 % and 16 % (Table 8, 9 and 10) depending on the qPCR platform applied, hence also below 25 %;
- the collaborative study (step 4 of the validation process) established that over the twelve participating laboratories at the level of 0.1 % related to mass fraction of GM-material the RSD_r of the method was 15 %, therefore also below 25 % and well in line with the previous data.

The outcome of the different steps is summarised Table 14.

Table 14. Precision of the event-specific method for quantitative detection of MON 95379 at or around 0.1 % level related to mass fractions of GM material.

Source	RSD_r %	GM %
Applicant's method optimisation	19 %	0.05 %*
Applicant's transferability study	13 %	0.085 %*
EURL GMFF tests	13-16 %	0.10 %
Collaborative study	15 %	0.10 %

*Expressed in copy number ratio

Based on the results of the EURL GMFF in-house verification and of the international collaborative study, it is concluded that the method RSD_r % is lower than 25 % at the level of 0.1 % related to mass fraction of GM material, hence the method meets the requirement laid down in Regulation (EU) No 619/2011.

7. Conclusion

The method provided by the applicant was validated in accordance to the EURL GMFF validation process, respecting all requirements of the relevant EU legislation and international standards for method validation.

This validation study confirmed that the method is applicable to the control samples provided by the applicant (see paragraph 4.1), in accordance with the requirements of Annex I-3.C.2 to Commission Regulation (EU) No 503/2013 and (EU) No 619/2011 and meets all method performance requirements established by the ENGL and the EURL GMFF. The method is therefore valid to be used for regulatory purposes, including the quantification of low-level presence of 0.1 % (m/m) of the GM event. It can be assumed that it is applicable to any appropriately extracted maize genomic DNA.

In any case, the user of the method is advised to verify the quality of the extracted genomic DNA in order to ensure that it is suitable for the subsequent PCR analysis. This is particularly relevant for more complex matrices of samples from food and feed products.

The validated method is described in detail as "Validated Method" at <http://gmo-crl.jrc.ec.europa.eu/StatusOfDossiers.aspx> and in Annex 1.

8. References

1. Regulation (EC) No 1829/2003 of the European Parliament and of the Council of 22 September 2003 on genetically modified food and feed.
2. Horwitz W. Protocol for the design, conduct and interpretation of method- performance studies, *Pure and Appl. Chem.* 1995; 67: 331-343.
3. International Standard (ISO) 5725-1, 1994. Accuracy (trueness and precision) of measurement methods and results. Part 1: General principles and definitions. International Organization for Standardization, Genève, Switzerland.
4. ISO 5725-1:1994/Cor 1:1998.
5. International Standard (ISO) 5725-2, 1994. Accuracy (trueness and precision) of measurement methods and results. Part 2: Basic method for the determination of repeatability and reproducibility of a standard measurement method. International Organization for Standardization, Genève, Switzerland.
6. ISO 5725-2:1994/Cor 1:2002.
7. Commission Implementing Regulation (EU) No 503/2013 of 3 April 2013 on Applications for Authorisation of Genetically Modified Food and Feed in Accordance with Regulation (EC) No

- 1829/2003 of the European Parliament and of the Council and amending Commission Regulations (EC) No 641/2004 and (EC) No 1981/2006.
8. Commission Regulation (EU) No 619/2011 of 24 June 2011 laying down the methods of sampling and analysis for the official control of feed as regards presence of genetically modified material for which an authorisation procedure is pending or the authorisation of which has expired.
 9. European Network of GMO Laboratories (ENGL). Definition of minimum performance requirements for analytical methods of GMO testing. 2015. <http://gmo-crl.jrc.ec.europa.eu/guidancedocs.htm>.
 10. Rogers S.O., Bendich A.J. Extraction of DNA from Milligram Amounts of Fresh Herbarium and Mummified Plant Tissue, *Plant Mol Biol Sci*, 1985; 69-76.
 11. Demeke T., Jenkins G.R. Influence of DNA extraction methods, PCR inhibitors and quantification methods on real-time PCR assay of biotechnology-derived traits. *Analytical and Bioanalytical Chemistry*, 2010; 396: 1977-1990.
 12. Peano C., Samson M.C., Palmieri L., Gulli M., Marmioli N. Qualitative and quantitative evaluation of the genomic DNA extracted from GMO and Non-GMO foodstuffs with four different extraction methods. *Journal of Agricultural and Food Chemistry*, 2004; 52: 6962-6968
 13. Bauer T., Weller P., Hammes W.P., Hertel C. The effect of processing parameters on DNA degradation in food. *European Food Research and Technology*, 2003; 217: 338-343
 14. Murray S.R., Butler R.C., Hardacre A.K., Timmerman-Vaughan G.M. Use of quantitative real-time PCR to estimate maize endogenous DNA degradation after cooking and extrusion or in food products. *Journal of Agricultural and Food Chemistry*, 2007; 55: 2231-2239
 15. Sedlackova T., Repiska G., Celec P., Szemes T., Minarik G. Fragmentation of DNA affects the accuracy of the DNA quantitation by the commonly used methods. *Biological Procedures Online*, 2013; 15: 1-9
 16. Plant DNA C-values Database, <http://data.kew.org/cvalues/>
 17. European Network of GMO Laboratories (ENGL). Verification of analytical methods for GMO testing when implementing interlaboratory validated methods. 2017. <http://gmo-crl.jrc.ec.europa.eu/ENGL/docs/WG-MV-Report-version-2.pdf>.
 18. Commission Implementing Regulation (EU) No 120/2014 of 7 February 2014 amending Regulation (EC) No 1981/2006 on detailed rules for the implementation of Article 32 of Regulation (EC) No 1829/2003 of the European Parliament and the Council as regards the Community reference laboratory for genetically modified organisms.

Annex 1: Event-specific Method for the Quantification of Maize MON 95379 by Real-time PCR

Validated Method

Method development:

Bayer Agriculture BV

1. General information and summary of the methodology

This protocol describes an event-specific real-time quantitative TaqMan® PCR (polymerase chain reaction) procedure for the determination of the relative content of maize event MON 95379 DNA to total maize DNA in a sample.

Template DNA extracted by means of suitable methods should be tested for quality and quantity prior to use in PCR assays. Tests for the presence of PCR inhibitors (e.g. monitor run of diluted series, use of DNA spikes) are also recommended to ensure suitability of the extracted DNA.

For the detection of GM event MON 95379, an 87 bp fragment of the region spanning the 3' insert-to-plant junction in maize-specific MON 95379 is amplified using specific primers. PCR products are measured during each cycle (real-time) by means of a target-specific oligonucleotide probe labelled with FAM (6-carboxyfluorescein) as reporter dye at its 5' end and TAMRA as quencher dye at its 3' end.

For the relative quantification of GM event MON 95379, a maize taxon-specific system amplifies a 79 bp fragment of a maize *high mobility group (hmg)* endogenous gene (Accession number: GenBank AJ131373.1), using *hmg* gene-specific primers and a *hmg* gene-specific probe labelled with FAM as reporter dye at its 5' end and TAMRA as quencher dye at its 3' end.

The measured fluorescence signal passes a threshold value after a certain number of cycles. This threshold cycle is called the "Cq" value. For quantification of the amount of MON 95379 DNA in a test sample, Cq values for the MON 95379 and the *hmg* systems are determined for the sample. Standard curves are then used to estimate the relative amount of MON 95379 DNA to total maize DNA.

2. Validation and performance characteristics

2.1 General

The method was optimised for suitable DNA extracted from genetically modified and conventional maize seeds and grain. Precision and trueness of the method were tested through an international collaborative ring trial using DNA samples at different GM contents.

2.2 Collaborative trial

The method was validated in an international collaborative study by the European Union Reference Laboratory for GM Food and Feed (EURL GMFF). The study was undertaken with twelve participating laboratories in March 2022.

A detailed validation report can be found at <http://gmo-crl.jrc.ec.europa.eu/StatusOfDossiers.aspx>.

2.3 Limit of detection (LOD)

According to the method developer, the relative LOD of the method is at least 5 copies of MON 95379 in 250 ng of total suitable maize DNA. The relative LOD was not assessed in the collaborative study.

2.4 Limit of quantification (LOQ)

According to the method developer, the relative LOQ of the method is at least 0.085 % (copies of MON 95379 per maize haploid genome copies) in 160 ng of total suitable maize DNA. The lowest relative GM content of the target sequence included in the collaborative trial was 0.1 % (mass fraction of GM-material).

2.5 Molecular specificity

The method exploits a unique DNA sequence in the region spanning the 3' insert-to-plant junction in maize MON 95379 and is therefore event-specific for the event MON 95379. This was confirmed in the validation study.

3. Procedure

3.1 General instructions and precautions

- The procedures require experience of working under sterile conditions.
- Laboratory organisation, e.g. "forward flow direction" during PCR-setup, should follow international guidelines, e.g. ISO 24276:2006.
- PCR reagents should be stored and handled in a separate room where no nucleic acids (with exception of PCR primers or probes) or DNA degrading or modifying enzymes have been handled previously. All handling of PCR reagents and controls requires dedicated equipment, especially pipettes.
- All the equipment should be sterilised prior to use and any residue of DNA should have been removed. All material used (e.g. vials, containers, pipette tips, etc.) must be suitable for PCR and molecular biology applications. They must be DNase-free, DNA-free, sterile and unable to adsorb protein or DNA.
- Filter pipette tips protected against aerosol should be used.
- Powder-free gloves should be used and changed regularly
- Laboratory benches and equipment should be cleaned periodically, with 10% sodium hypochlorite solution (bleach).
- Pipettes should be checked regularly for precision and calibrated, if necessary.

- All handling steps, unless specified otherwise, should be carried out at room temperature.
- In order to avoid repeated freeze/thaw cycles aliquots should be prepared.

3.2 Real-time PCR for quantitative analysis of maize event MON 95379

3.2.1 General

The real-time PCR set-up for the taxon (*hmg*) and the GMO (event MON 95379) target sequences are carried out in separate vials. Multiplex qPCR (using differential fluorescent labels for the probes) has not been tested or validated by the EURL GMFF.

The method is developed for a total volume of 25 µL per reaction mixture for the GM (event MON 95379) and the taxon (*hmg*) assay with the reagents as listed in Table 2 and Table 3.

3.2.2 Calibration

The calibration curves have to be established on at least five samples. The first point of the calibration curve (S1) should be established for a sample containing 10 % maize MON 95379 DNA in a total of 250 ng of maize DNA (corresponding to 91575 maize haploid genome copies with one haploid genome assumed to correspond to 2.73 pg of maize genomic DNA)⁽¹⁾. Standards S2 to S5 are prepared by serial dilutions (dilution factor 4 for samples S2-S4 and dilution factor 5 for standard S5) according to Table 1 below.

Table 1. Copy number values of the standard curve samples

Sample code	S1	S2	S3	S4	S5
Total amount of maize DNA in reaction (ng)	250	62	16	3.9	0.78
Maize haploid genome copies	91575	22894	5723	1431	286
MON 95379 copies	9158	2289	572	143	29

A calibration curve is to be produced by plotting the C_q values against the logarithm of the target copy number for the calibration points. This can be done by means of spreadsheet software, e.g. Microsoft Excel, or directly by options available with the software.

The copy number measured for each unknown sample DNA is obtained by interpolation from the standard curves.

3.2.3 Real-time PCR set-up

1. Thaw, mix and centrifuge the components needed for the run. Keep thawed reagents on ice.
2. In two tubes on ice, add the components in the order mentioned below (except DNA) to prepare the reaction mixes for the MON 95379 maize specific system (Table 2) and the *hmg* reference gene system (Table 3). Please note that additional volume is included in the total to cover pipetting variability due to the viscosity of the solution.

Table 2. Amplification reaction mixture in the final volume/concentration per reaction well for the MON 95379 assay.

Component	Final concentration	µL/reaction
TaqMan® Universal PCR Master Mix (2x)	1x	12.5
MON 95379 primer 1 (10 µM)	400 nM	1.0
MON 95379 primer 2 (10 µM)	400 nM	1.0
MON 95379 probe* (10 µM)	200 nM	0.5
Nuclease free water	-	6.0
DNA	-	4
Total reaction volume:		25 µL

*probe labelled with 6-FAM at its 5'-end and TAMRA at its 3'-end

Table 3. Amplification reaction mixture in the final volume/concentration per reaction well for the maize *hmg* assay.

Component	Final concentration	µL/reaction
TaqMan® Universal PCR Master Mix (2x)	1x	12.5
<i>hmg</i> primer 1 (10 µM)	300 nM	0.75
<i>hmg</i> primer 2 (10 µM)	300 nM	0.75
<i>hmg</i> probe* (10 µM)	160 nM	0.40
Nuclease free water	-	6.6
DNA	-	4
Total reaction volume:		25 µL

*probe labelled with 6-FAM at its 5'-end and TAMRA at its 3'-end

3. Mix well and centrifuge briefly.
4. Prepare two 0.5 mL reaction tubes (one for the maize MON 95379 and one for the *hmg* system) for each DNA sample to be tested (standard curve samples, unknown samples and control samples).

5. Add into each reaction tube the amount of reaction mix for 3.5 PCR repetitions (73.5 μ L for the MON 95379 maize system and 73.5 μ L for the *hmg* system). Add to each tube the correct amount of DNA for 3.5 PCR repetitions (14 μ L DNA). The volume for the additional 0.5 repetition will ensure adequate volume when loading the samples. Vortex each tube for approx. 10 seconds. This step is mandatory to reduce to a minimum the variability among the repetitions of each sample.
6. Spin down the tubes. Aliquot 25 μ L for the MON 95379 system and for the *hmg* reference system in each well.
7. Place an optical cover on the reaction plate and briefly centrifuge the plate.
8. Place the reaction plate in the real-time PCR apparatus (possibly apply a compression pad, depending on the model), according to the manufacturer's instructions and your Standard Operating Procedures and start the run.
9. Select 6-FAM as reporter dye for the MON 95379 and 6-FAM for the *hmg* reference system. Define TAMRA or non-fluorescent as quencher dye for MON 95379 specific system and for *hmg* reference system. Select ROX (6-carboxy-X-rhodamine) as the passive reference dye. Enter the correct reaction volume (25 μ L).
10. Run the PCR with the cycling program described in Table 4.

Table 4. Cycling program for MON 95379 / *hmg* assays.

Step	Stage	T ($^{\circ}$ C)	Time (s)	Acquisition	Cycles	
1	UNG*	50	120	No	1	
2	Initial denaturation	95	600	No	1	
3	Amplification	Denaturation	95	15	No	45
		Annealing & Extension	60	60	Yes	

*UNG: Uracil-N-glycosylase

3.3 Data analysis

After the real-time PCR, analyse the run following the procedure below:

- a) Set the threshold following the automatic or the manual mode. In the manual mode, display the amplification curves of the event specific assay in logarithmic mode. Locate the threshold line in the area where the amplification profiles are parallel (exponential phase of PCR) and where there is no "fork effect" between repetitions of the same sample. Press the "update" button to ensure changes affect Cq values (only needed for some analysis software). Switch to the linear view mode by clicking on the Y axis of the amplification plot and check that the threshold previously set falls within the exponential phase of the curves.
- b) Set the baseline following the automatic or the manual mode. In the manual mode: determine the cycle number at which the threshold line crosses the first amplification curve and set the baseline three cycles before that value (e.g. earliest Cq = 25, set the baseline crossing at $Cq = 25 - 3 = 22$).
- c) Save the settings.
- d) Repeat the procedure described in a), b) and c) on the amplification plots of the taxon specific system.
- e) Save the settings and export all the data for further calculations.

3.4 Calculation of results

After having defined a threshold value within the logarithmic phase of amplification as described above, the instrument's software calculates the Cq values for each reaction.

The standard curves are generated for both the *hmg* and the MON 95379 specific assays by plotting the Cq values measured for the calibration points against the logarithm of the DNA copy numbers and by fitting a linear regression line into these data.

Thereafter, the standard curves are used to estimate the DNA copy number in the unknown samples.

To obtain the percentage value of event MON 95379 DNA in the unknown sample, the MON 95379 copy number is divided by the copy number of the maize endogenous gene *hmg* and multiplied by 100 ($GM\% = \text{MON 95379}/hmg \times 100$).

4. Equipment and Materials

4.1 Equipment

- Real-time PCR instrument for plastic reaction vessels (glass capillaries are not recommended for the described buffer composition) and appropriate analysis software
- 96-well reaction plates

- Optical caps/adhesion covers
- Microcentrifuge
- Micropipettes
- Standard bench top centrifuge with rotor or standard microfuge fit for 0.5 mL reaction tubes, centrifuge for 96-Well reaction plates
- Vortex
- Racks for reaction tubes, also cooled
- 0.5, 1.5 mL and 5 or 15 mL DNase free reaction tubes

4.2 Reagents

- TaqMan® Universal PCR Master Mix. Applied Biosystems Part No 4318157.

4.3 Primers and Probes

Table 5. Primers and probes for the MON 95379 and *hmg* methods

	Name	DNA Sequence (5' to 3')	Length (nt)
<i>MON 95379</i>			
Forward primer	MON 95379 primer 1	CCA AGA AGA ACG ATT GGC AAA C	22
Reverse primer	MON 95379 primer 2	GGC ACA GGC ACG CCT CTG	18
Probe	MON 95379 probe	6-FAM-ATG GGT ATT ATG GGT AGG CAC ATG GGA ATA TAG-TAMRA	33
<i>hmg</i>			
Forward primer	<i>hmg</i> primer 1	TTG GAC TAG AAA TCT CGT GCT GA	23
Reverse primer	<i>hmg</i> primer 2	GCT ACA TAG GGA GCC TTG TCC T	22
Probe	<i>hmg</i> probe	6-FAM-CAA TCC ACA CAA ACG CAC GCG TA-TAMRA	23

5. References

1. Plant DNA C-values Database. Royal Botanic Gardens, Kew, <http://data.kew.org/cvalues/>

The European Commission's science and knowledge service

Joint Research Centre

JRC Mission

As the science and knowledge service of the European Commission, the Joint Research Centre's mission is to support EU policies with independent evidence throughout the whole policy cycle.



EU Science Hub
joint-research-centre.ec.europa.eu

 @EU_ScienceHub

 EU Science Hub - Joint Research Centre

 EU Science, Research and Innovation

 EU Science Hub

 EU Science